



FIGURE 297e-19 Transesophageal echocardiogram showing sizing balloon (*left*) and no flow (*right*) across the atrial septal defect.

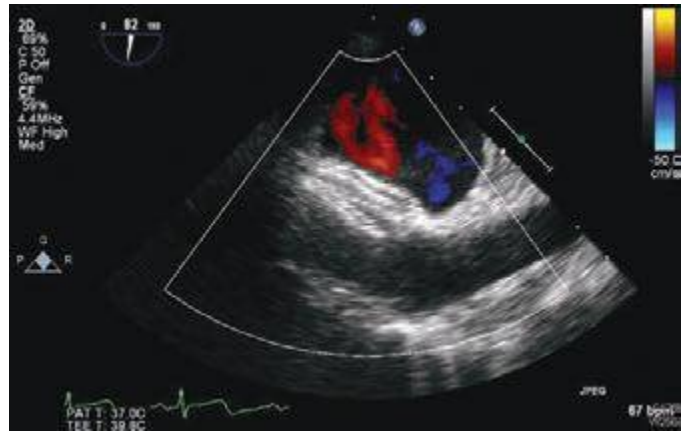


FIGURE 297e-20 Amplatzer® septal occluder in place (*left*). There is no blood flow across the device (*right*).

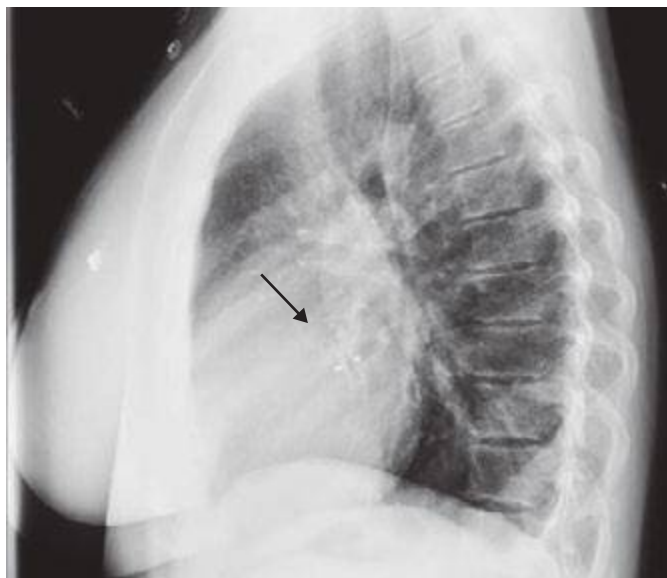


FIGURE 297e-21 Postprocedure lateral chest x-ray showing the Amplatzer® septal occluder in place.